


# EC200 Electrochemical Sensor Controller Manual

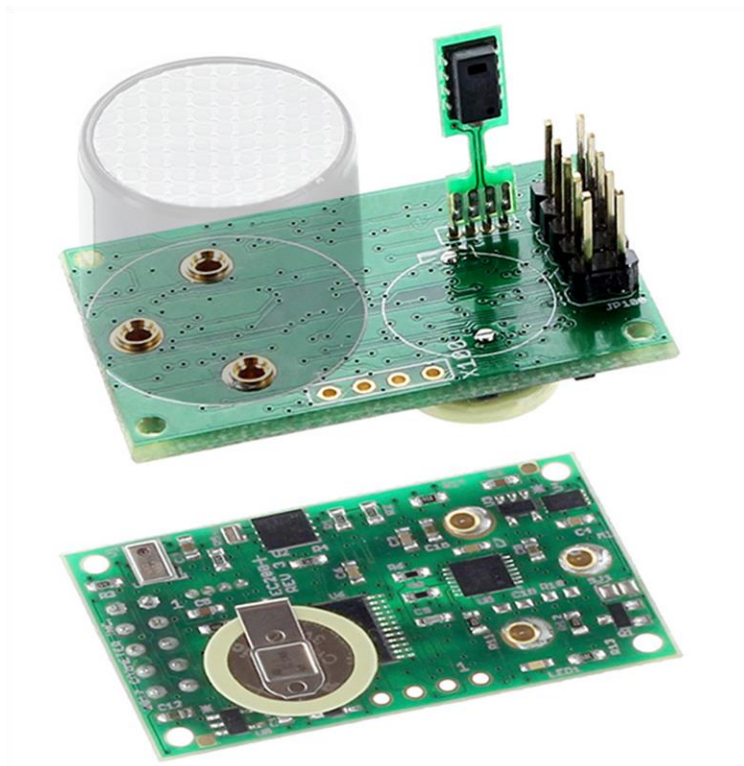

 **CO2Meter.com**

The information in this document is protected under applicable federal law as an unpublished work and is confidential and proprietary to Co2Meter Inc. Its use, disclosure, reproduction, or publication, in whole or in part, without the express prior written consent of Co2Meter, Inc. is prohibited.

© 2014-2018 CO2METER, INC. All Rights Reserved.

## Document History

<b>Date</b>	<b>Revision</b>	<b>Description</b>
<b>14 August, 2014</b>	A	Initial Release
<b>18 February, 2015</b>	B	Version 2 Firmware
<b>11 May, 2017</b>	C	Version 3 Firmware
<b>12 September, 2017</b>	D	Final Draft for Review
<b>10 October, 2017</b>	E	Publish
<b>13 October, 2017</b>	F	Added dimensional drawing
<b>14 February, 2018</b>	G	Firmware EC200v3b008. Add # command, Add J for AUX voltage logging. Scaling for PWM and Analog outputs. Clarification and elaboration.
<b>20 February, 2018</b>	H	Detail on Parameter 3
<b>3 March, 2018</b>	J	Firmware EC200v3b008 Add “[“command Correction and clarifications
<b>13 March, 2018</b>	K	Firmware EC200v3b010. Correct “z” and “G” command. Streaming and RS485 mutual exclusive
<b>14 March, 2018</b>	L	Firmware EC200v3b11. Add select on power up RS485.
<b>19 March 2018</b>	M	Firmware EC200v3b13 doc; Correction and addition; gas types, error codes.
<b>20 March 2018</b>	N	Firmware EC200v3b16. Corrections fix mask function error. Doc Pressure compensation flag
<b>April 6 2018</b>	O	Firmware EC200v3b17 clarification data logging, calibration procedure, temperature compensation flag



## Table of Contents

DOCUMENT HISTORY.....	II
<b>INTRODUCTION.....</b>	<b>7</b>
ABOUT THIS MANUAL.....	7
<b>CHAPTER 1 : OVERVIEW.....</b>	<b>8</b>
GENERAL.....	8
MEASUREMENTS .....	8
Unfiltered Voltage ( <i>v</i> ).....	8
Filtered Voltage ( <i>V</i> ).....	8
Unfiltered Uncompensated Concentration ( <i>D</i> ).....	8
Unfiltered Concentration ( <i>z</i> ).....	8
Filtered Concentration ( <i>Z</i> ) .....	8
Temperature ( <i>T</i> ).....	8
Humidity ( <i>H</i> ).....	9
Barometric Pressure ( <i>B</i> ).....	9
Dimensional Drawing.....	9
<b>CHAPTER 2 : COMMUNICATIONS INTERFACE.....</b>	<b>10</b>
GENERAL.....	10
PHYSICAL CONNECTIONS .....	10
CONNECTOR ASSIGNMENTS.....	10
RS485 INPUT .....	11
PWM OUTPUT.....	11
ANALOG OUTPUT .....	11
ANALOG INPUT (DIFFERENTIAL) .....	11
LINK LEVEL PARAMETERS.....	11
TTL PROTOCOL.....	11
MODES .....	11
COMMANDS .....	12
Error codes:.....	12
<i>B</i> Command – Get Barometric Pressure.....	13
<i>b</i> Command – Get Barometric Pressure.....	13
<i>C</i> Command – Set Current Date and Time .....	13
<i>c</i> Command – Get Current Date and Time .....	14
<i>G</i> Command – Get Sensor Type.....	14
<i>H</i> Command – Get Relative Humidity.....	14
<i>J</i> Command – Get Auxiliary Analog Input.....	15
<i>K</i> Command – Set Communications Mode .....	15
<i>M</i> Command – Set Output Fields .....	16
<i>P</i> Command – Set Parameter to Value .....	17
<i>p</i> Command – Get Parameter Value .....	17
<i>Q</i> Command – Get Readings.....	17
<i>R</i> Command – Read Log Memory.....	18
<i>r</i> Command – Erase Log Memory.....	18
<i>T</i> Command – Get Temperature .....	19
<i>t</i> Command – Raw Temperature voltage from Barometer.....	19
<i>U</i> Command – Zero Calibrate.....	19
<i>u</i> Command – Set Zero Calibration Point.....	20

<i>V Command – Get Filtered voltage</i> .....	20
<i>v Command – Get Unfiltered voltage</i> .....	20
<i>W Command – Write Current Parameter Values to Flash</i> .....	21
<i>w Command – Reset Parameters to Manufacturing Defaults</i> .....	21
<i>X Command – Calibrate to specified concentration</i> .....	21
<i>x Command – Reserved for Factory Use</i> .....	22
<i>Y Command – Report Device Identification</i> .....	22
<i>Z Command – Get Filtered Gas Concentration</i> .....	22
<i>z Command – Get Unfiltered Gas Concentration</i> .....	22
<i>. Command – Get Multiplier</i> .....	23
<i>[ Command – reload AFE and restart</i> .....	23
<b>RS 485 INTERFACE COMMANDS</b> .....	23
<i>! Command – Select Device</i> .....	24
<i># Command– Restart</i> .....	25
<b>CHAPTER 3 : CONFIGURATION</b> .....	<b>26</b>
GENERAL.....	26
PARAMETER SUMMARY.....	26
<i>Checksum (0)</i> .....	27
<i>Output Mode (1)</i> .....	27
<i>Log Mode (2)</i> .....	27
<i>AFE Configuration (3)</i> .....	27
<i>Configuration Option Word (4)</i> .....	27
<i>Log Interval (5)</i> .....	28
<i>Gas Type (6)</i> .....	28
<i>Zero Calibration (7)</i> .....	28
<i>Calibration at Reference (8)</i> .....	28
<i>Calibration Concentration (9)</i> .....	28
<i>PWM Full Scale (10)</i> .....	28
<i>Analog Full Scale (11)</i> .....	29
<i>Multiplier (12)</i> .....	29
<i>Feature Configuration (13)</i> .....	29
<i>Temperature Compensation Values (16-31)</i> .....	30
<b>CHAPTER 4 : CALIBRATION</b> .....	<b>31</b>
GENERAL.....	31
BASIC CALIBRATION.....	31
RECOMMENDATION HANDLING, STORAGE AND CALIBRATION;.....	31
<b>CHAPTER 5 : LOGGING</b> .....	<b>33</b>
GENERAL.....	33
LOG BLOCKS.....	33
SHORT BLOCKS.....	33
LOG CAPACITY.....	33
DATE/TIME FORMAT.....	33
BLOCK HEADER DECODING START TIME EXAMPLE;.....	34
EXAMPLE OF LOGGING OPERATION, PARTIAL BLOCK AND START RESTART;.....	34
<b>SUPPORT</b> .....	<b>37</b>
WARRANTY.....	37
LIABILITY.....	37

RETURNS.....	37
CONTACT US .....	38

## Introduction

### About this Manual

This document is a technical reference for the CO2Meter.com EC200 Electrochemical Sensor Controller. It provides the information necessary to use the sensor controller as well as information about configuring the controller for various applications.

## Chapter 1 : Overview

### General

The EC200 Sensor Controller is a high performance low power controller supporting a wide variety of 20mm electro-chemical plug-in gas sensor cells. The controller supplies the necessary interface to the gas sensor cell and converts the sensor output current to a voltage that is measured by a high-resolution analog to digital converter. This digital voltage is then corrected and compensated for temperature and pressure by a microcontroller to produce an accurate gas concentration measured in ppm (parts per million). Measurements are available at the serial interface and/or can be logged to non-volatile storage for later retrieval.

In typical applications the sensor samples once per second and filters readings over 8 seconds. The sample interval is user configurable.

### Measurements

The EC200 makes several measurements, typically once per second. Any or all of these are available through the streaming interface as described in Chapter 2. In the descriptions below, the letter in parenthesis is that used to report the value on the communication interface.

#### *Unfiltered Voltage (v)*

This is voltage from the analog front-end circuit. This voltage is directly proportional to the current from the electrochemical gas sensor cell. The current to voltage transfer function depends on the configuration for the particular sensor in use.

#### *Filtered Voltage (V)*

This is the voltage from the analog front-end passed through a low pass filter that removes short-term (seconds) disturbances.

#### *Unfiltered Uncompensated Concentration (D)*

This is the computed unfiltered gas concentration prior to compensation for temperature and pressure.

#### *Unfiltered Concentration (z)*

This is the computed unfiltered gas concentration compensated for temperature. The temperature compensation is performed using 5C degree values determined during factory calibration. Linear interpolation is used between calibration values.

#### *Filtered Concentration (Z)*

This is the filtered gas concentration compensated for temperature and temperature. This is the primary measurement made by the device.

#### *Temperature (T)*

This is the temperature reading from temperature/humidity sensor device.




### Humidity (H)

This is the Relative Humidity reading from the temperature/humidity sensor device.

### Barometric Pressure (B)

For models equipped with a barometric sensor, this is the barometric pressure. This value is corrected by the microprocessor for linearity and temperature using values determined during manufacturing of the sensor. Barometric Pressure is valid only in the range from 500 – 1150 millibar.

### Dimensional Drawing

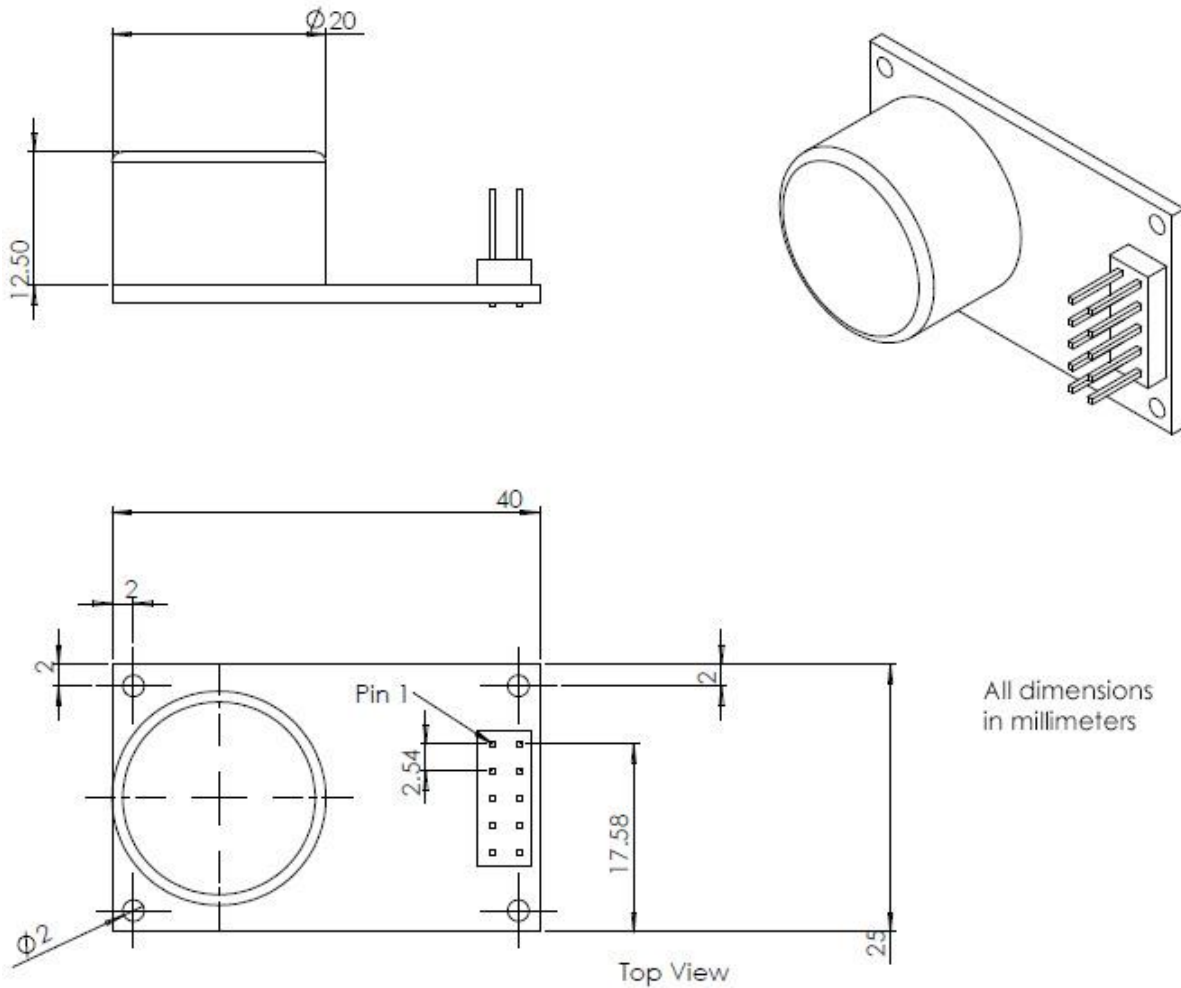

## Chapter 2 : Communications Interface

### General

The EC200 communicates with a host system through a UART interface using either CMOS/TTL Rx and Tx or Differential RS485. The EC200 is a 3V system. The Rx input, however, is fault-tolerant to 5V and will generally interoperate with 3V to 5V systems. The EC200 also has a half-duplex RS485 interface that allows operation over long cables. The RS485 is enabled when Pin 2 is low at power up.


When RS485 is enabled (Pin 2 low at power up), the Communication Interface can be operated in either single sensor or multiple sensor mode. Multiple sensor mode permits up to 31 sensors to be multi-dropped on the same differential pair.

### Physical Connections

The EC200 uses a 10 pin (2x5) header with 0.1 inch centers. When viewed from the sensor side with the connector to the left side of the board, Pin 1 is the lower right pin of the header.

### Connector Assignments

Pin	Function	Pin	Function
1	Power and Signal Return	2	Select: PWM /RS485
3	+3 to +5.5V Power	4	AUX Analog -
5	Rx (Input to Sensor)	6	AUX Analog +
7	Tx (Output from Sensor)	8	RS485 A (Data -)
9	Analog Output ( 0 - 3V)	10	RS485 B (Data +)

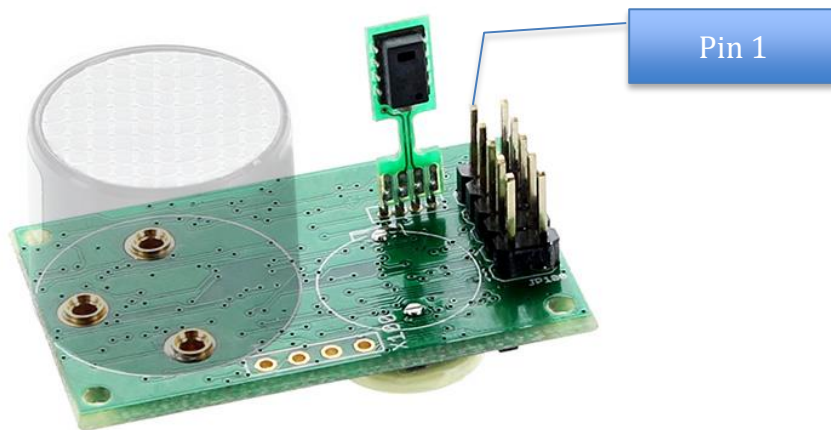

### RS485 Input

If ground is applied to Pin 2 (Select: PWM/ RS485) at power up, the RS485 interface is selected. The RS485 Interface will be used for both transmit and receive. (TTL level TX output will also occur on pin 7). Note that RS485 is two wire half duplex. The EC200 is normally listening and enables transmit only when transmitting a reply to the host system.

### PWM Output

If the Select/PWM output is open (or high) at power up, the TTL serial interface is selected and PWM is supplied from pin 2, **if** additionally; Configuration Option word register 4, Bit 14 (16384) is set PWM operation is enabled.

### Analog Output

Pin 9 can be configured as an analog output with a full scale range from 0.00 to 3.00V. The output is derived from a 1ms PWM filtered by a restoration filter consisting of a 10k resistor and 1uF capacitor. The output impedance is approximately 10K. Note that the impedance of the input will reduce the maximum output voltage to approximately  $3.0V * Z / (Z + 10k)$ . For example, with an input impedance of 50K the full scale output will be  $3.0 * 50k / 60k = 2.5$ Volts.

### Analog Input (Differential)

Pins 4 and 6 provide an auxiliary differential analog input. The full scale voltage range between inputs is -1.0V to +1V. The voltage on either pin with respect to ground must be in the range from -1.0V to +3V. NO PROTECTION IS PROVIDED FOR INPUT OVERVOLTAGE.

The typical singled ended input impedance (either pin to ground) is 200kOhm. The differential input impedance (between pins) is 300kOhm minimum 400kOhm typical.

The auxiliary analog input value is available via command "J".

### Link Level Parameters

The line-level communications parameters are asynchronous 9600 baud, 8 bits, no parity, and a single stop bit, CMOS logic level 3.3 volt interface, communications is full duplex. For the RS485 interface, communications is half duplex.

### TTL Protocol

The host and the controller exchange lines of data. Each line of data to and from the controller is terminated by carriage linefeed (CR LF), i.e. ASCII 0x0d, 0x0a.

The controller always responds to each line. If the line contains a valid command, the controller acts on the command and returns a response. If the line is not recognized as a valid command the controller returns an error response.

### Modes

The controller operates in one of two modes, polled or streaming. In polled mode the controller is silent except in response to a command. In streaming mode, the controller

reports measurements at intervals of one second (or more) as determined by configuration.

With the CMOS interface, commands may be sent at any time and the controller will continue to stream measurements until the entire command is received. With the RS485 interface, the half-duplex nature of the interface requires that the host is host transmit only in the interval between streamed measurements or responses from the controller.

At power up the controller enters polled or streaming mode depending on configuration. The mode can be temporarily changed with the K command.

Except during calibration, the controller enters a low power state between measurements. The controller will awaken with the falling edge of any data transmission from the host.

### Commands

Each of the commands supported by the controller is described in the following. Each command consists of a single letter optionally followed by a space and one or two numeric fields separated by a single space. All other letter values not listed are reserved and should not be sent.

The controller always outputs numeric values as 5 decimal digits with leading zeroes if necessary. The controller accepts numeric values with 1 to 5 digits in the range from 0 to 65535.

The controller always responds to a command. The response to a valid and properly formatted command will begin with the command letter except in the case of the “Q” command (which returns the exact line that will be send during streaming). If the command is not valid and properly formatted, the response will be an error code.

### Error codes:

- 1 – Unrecognized Command
- 2 – Improper Format
- 3 – Improper Value
- 4 – Invalid Date String
- 5 – Write Error
- 6 – Read Error
- 7 – Bad Parameter
- 8 – Value already set
- 9 – Command failed
- 10 – Command not implemented
- 11 – Not configured

Error responses begin with the letter “E” following by a space and the 5 digit error number. For example, if a command with an invalid command letter is sent the response will be:

```
E 00003<cr><lf>
```

### ***B Command – Get Barometric Pressure***

This command gets the barometric pressure. The value is in tenths of millibars in the range from 500 – 1150, i.e. the values returned will be in the range 5000 to 11500.

Example Request:

```
B<cr><lf>
```

Example Response:

```
B 10156<cr><lf>
```

This response indicates a barometric pressure of 1015.6 millibars.

### ***b Command – Get Barometric Pressure***

This command gets the barometric pressure ADC value is in tenths of millibars referenced but not compensated .

Example Request:

```
b<cr><lf>
```

Example Response:

```
b 26688<cr><lf>
```

### ***C Command – Set Current Date and Time***

This command is used to set the Date and Time for the real-time clock calendar. This is used for logging. The date format is ISO 8601 format, i.e. YYYY-MM-DDTHH:MM:SS where the hour is based on a 24 hour clock. The format must be exact. When using a terminal, it is usually best to do a “c” command first to see the correct format.

Example Request:

```
C 2014-08-06T13:10:22<cr><lf>
```

Example Response:

```
c 2014-08-06T13:10:22<cr><lf>
```

### ***c Command – Get Current Date and Time***

This command is used to get the current date and time.

Example Request:

```
c<cr><lf>
```

Example Response:

```
c 2014-08-06T13:10:22<cr><lf>
```

### ***G Command – Get Sensor Type***

This command is used to obtain an abbreviation for the type of sensor and its full span range. The value returned is a concentration followed by 4-character string with trailing spaces. Note that the concentration must be scaled according to the scale factor returned by the "." command. Values include "CO", "O2", "H2S", "NO ", "SO2 ", "CL2 ", "SO2 ", "ET ", "H2 ", "HCL", "SOH ", "HCN ", "PH3 ", and "NO2 ".

Example Request:

```
G <cr><lf>
```

Example Response:

```
G 01000 CO<space><space><cr><lf>
```

Assuming that the scale factor from "." is 1, the above response indicates that the controller is configured for a 1000ppm Carbon Monoxide sensor.

### ***H Command – Get Relative Humidity***

This command is used to get the relative humidity. The value is supplied in tenths of percent relative humidity.

Example Request:

```
H<cr><lf>
```

Example Response:

```
H 00452<cr><lf>
```

### ***J Command – Get Auxiliary Analog Input***

This command is used to get the voltage presented at the analog input. As this the input is differential, the value is presented in offset bipolar form. 32768 corresponds to 0. Values above 32768 are positive voltages. Values less than 32768 are negative values. The signed value can be obtained by subtracting 32768 from the value. For example, a value of 65000 is +32232. A value of 2000 is -30768. The result must be divided by 32768 to get the percentage of the full scale range which is plus or minus 1 volt.

Example Request:

```
J<cr><lf>
```

Example Response:

```
J 34000<cr><lf>
```

This value is converted to a voltage as  $(34000-32768)*1.0/32768 = 0.0376$  volts. An example with a negative value is:

Example Response:

```
J 30000<cr><lf>
```

This value is converted to voltage as  $(30000-32768)*1.0/32768 = -0.0845$  volts.

### ***K Command – Set Communications Mode***

This command is used to the communications the communication mode. A value of 1 sets the mode to streaming and a value of 2 sets to the mode to polled. The response is a “K” followed by the new mode. Note: a mode value of 0 is also accepted and behave exactly like Mode 2.

Example Request:

```
K 2<cr><lf>
```

Example Response:

```
K 00001<cr><lf>
```

### M Command – Set Output Fields

This command is used to the fields that are sent in streaming mode, or in response to the “Q” command. A single 16-bit number is used to set the fields in accordance with the following table.

Measurement	ID	Mask Value	Description
Reserved		32768	
Reserved		16384	
Barometric Pressure	B	8192	Barometric Pressure
Relative Humidity	H	4096	Relative Humidity
Uncompensated Gas	D	2048	Uncompensated Unfiltered Gas Concentration
Raw ADC Value	d	1024	Raw ADC Value from analog front-end
Reserved	-	512	
Auxiliary Voltage	J	256	Auxiliary Voltage differential input.
Filtered Voltage	V	128	Filtered Voltage from analog front-end
Temperature	T	64	Temperature from RH Sensor
Temperature ADC	t	32	Raw Barometric Sensor Temp Value
Pressure ADC	b	16	Raw Barometric Pressure ADC Value
Unfiltered Voltage	v	8	Unfiltered Voltage from analog front-end
Filtered Gas	Z	4	Filtered and Compensated Gas Concentration
Unfiltered Gas	z	2	Unfiltered Compensated Gas Concentration
Reserved		1	

To set the output format add together the “Mask Values” from the above table for those readings that you wish to include in the output. For example, if want to display Filtered Gas “Z” (4) and Temperature “T” (64) add the two mask values to get 68 and use this as the value for the M command.

Example Request:

```
M 68<cr><lf>
```

Example Response:

```
M 00068<cr><lf>
```

A subsequent Q command will then give us an output as follows:



Example Request:

```
Q<cr><lf>
```

Example Response:

```
Z 00004 T 01254<cr><lf>
```

The output of the Q command is the same output that will with each line when streaming is on.

If 0 or an reserved bit is selected all fields will be reported on “Q” command or streaming mode.

#### ***P Command – Set Parameter to Value***

This command is used to set the value of a parameter. The command requires the address of the parameter (0 – 31) and the new value.

Example Request:

```
P 4 10<cr><lf>
```

Example Response:

```
P 4 10<cr><lf>
```

#### ***p Command – Get Parameter Value***

This command is used to get the current value for selected parameter 0-31.

Example Request:

```
p 4<cr><lf>
```

Example Response:

```
p 4<cr><lf>
```

#### ***Q Command – Get Readings***

This command is used to get the readings that would be send in streaming mode. The format of the reply depends on current output format as set by the “M” command.

Example Request:

```
Q<cr><lf>
```

Example Response:

```
Z 00004 T 01254 H 00455 B 10149<cr><lf>
```

The above response indicates a gas concentration of 4ppm, a temperature of 25.4 degrees C, a relative humidity of 45.5% and barometric pressure of 1014.9 millibar.

### *R Command – Read Log Memory*

This command is used to read the EEROM memory used for logging. Memory is organized as 32768, 16-bit words. Each word has a decimal value range from 00000 to 65535.

The R command requires two parameters. The first is an Address in the range from 0 to 32767. The second parameter is a word count in the range of 1 to 8.

The memory is organized in 256 word blocks and each read is confined to a single block. If a read operation extends across a block, the read operation wraps around to the start of that block. Wraparounds are avoided by always accessing data on an 16-byte boundary, i.e. with an address that is evenly divisible by 16.

Example Request:

```
R 32 8<cr><lf>
```

Example Response:

```
R 00514 00514 00514 00514 00514 00514 00514 00514  
<cr><lf>
```

### *r Command – Erase Log Memory*

This command is used to erase all of log memory. After issuing this command the user should wait at least 5 seconds before issuing another command that accesses log memory. Note that when the controller responds to this command it will complete the erase operation in the background and then return to low power mode.

Example Request:

```
r 12345<cr><lf>
```

Example Response:

```
r <cr><lf>
```

### ***T Command – Get Temperature***

This command is used to obtain the current temperature. The response is in tenths of a degree C using an “excess 1000” notation. This always results in a positive value. For example, the reading 01250 corresponds to 25.0C, the reading 01000 corresponds to 0.0C and the reading 00970 corresponds to -3.0C. In other words, just subtract 1000 and the result will be the temperature in signed tenths of degrees C.

Example Request:

```
T<cr><lf>
```

Example Response:

```
T 01275<cr><lf>
```

This response indicates a current temperature of 27.5 Degrees C.

### ***t Command – Raw Temperature voltage from Barometer***

This command is used to obtain the raw temperature from the barometer. It is a signed integer proportional the temperature the barometer die is sensing.

Example Request:

```
t<cr><lf>
```

Example Response:

```
t 01275<cr><lf>
```

This response indicates a current temperature of 27.5 Degrees C.

### ***U Command – Zero Calibrate***

This command is used to set the zero point for the sensor. Calibration is normally performed using Nitrogen gas at 26C plus or minus 1C as further discussed in Chapter 4.

Example Request:

```
U<cr><lf>
```

Example Response:

```
U 11192<cr><lf>
```

The response to the command is the numeric value corresponding to the zero point. This value can be used with a subsequent “u” command to restore the zero point.

#### ***u Command – Set Zero Calibration Point***

This command is used to manual set the zero point to a value from a previous calibration.

Example Request:

```
u 11192<cr><lf>
```

Example Response:

```
U 11192<cr><lf>
```

#### ***V Command – Get Filtered voltage.***

This command is used to obtain the filter voltage from the electro chemical sensor. Value is in millivolts.

Example Request:

```
V<cr><lf>
```

Example Response:

```
V 01275<cr><lf>
```

This response indicates a voltage of +1275 mV.

#### ***v Command – Get Unfiltered voltage.***

This command is used to obtain the Unfilter voltage from the electro chemical sensor . Value is in millivolts.

Example Request:

```
v<cr><lf>
```

Example Response:

```
v 01275<cr><lf>
```

This response indicates a voltage of +1275 mV.

### *W Command – Write Current Parameter Values to Flash*

This command is used to write the current set of 32 parameter values to flash. By design, parameters that are changed are **not** automatically written to non-volatile memory until a W command is issued or a calibration is performed. The W command calculates the check sum (parameter 0) for parameters 1-31 parameter then writes parameters 0-31 to non-volatile memory

Example Request:

```
W<cr><lf>
```

Example Response:

```
W<cr><lf>
```

### *w Command – Reset Parameters to Manufacturing Defaults*

This command is used to restore all parameters to their default. This will wipe out any calibration that has been performed. The unlock code of “12345” is required to prevent accidentally invoking this command. All 32 parameters will be written.

The first parameter provides a numeric sensor type which determines the default values. This should be 1 for CO and 2 for O2.

Example Request:

```
w 1 12345<cr><lf>
```

Example Response:

```
w 1<cr><lf>
```

### *X Command – Calibrate to specified concentration*

This command is used to calibrate the sensor using a gas of known calibration. The sensor must have been previously zeroed. The calibration gas should be at 25 to 27 degree C. The gas reading must be stable prior to issuing this command.

Example Request:

```
X 500<cr><lf>
```

Example Response:

```
X 16076<cr><lf>
```

Assuming a sensor cell with a 1ppm resolution, this example sets the calibration for 500 ppm. The returned value of 16076 is the filtered ADC value at the calibration point.

#### *x Command – Reserved for Factory Use*

This command is reserved for factory use.

#### *Y Command – Report Device Identification*

This command is used to obtain information about the device.

Example Request:

```
Y<cr><lf>
```

Example Response:

```
Y CO2METER EC200 SN 00080 VER 03 BUILD 008<cr><lf>
```

#### *Z Command – Get Filtered Gas Concentration*

This command is used to obtain the filtered and compensated gas concentration. The 5-digit value returned must be multiplied by the multiplier value to arrive at ppm. For a multiplier of 1, the value will be actual ppm.

Example Request:

```
Z<cr><lf>
```

Example Response:

```
Z 00004<cr><lf>
```

This example response would be returned for a sensor with a resolution of 1ppm that is presently seeing a gas concentration of 4ppm.

#### *z Command – Get Unfiltered Gas Concentration*

This command is used to obtain the unfiltered (i.e. current) gas concentration.

Example Request:

```
z<cr><lf>
```

Example Response:

```
z 0003<cr><lf>
```

This example response would be returned for a sensor with a resolution of 1ppm that is seeing a gas concentration of 3ppm.

#### **. Command – Get Multiplier**

This command returns the multiplier that should be applied to the gas concentration reading to arrive at ppm. This will generally be 0, 1, 10, or 100 depending on the range of the sensor. Note that 0 is used for a multiplier of 0.1, i.e. 1/10<sup>th</sup> ppm.

Example Request:

```
.<cr><lf>
```

Example Response:

```
. 00001<cr><lf>
```

#### **[ Command – reload AFE and restart**

Reloads the constant from parameter registers used to operate 91000 and restart 91000 used when adjusting offset, bias, and gains.

Example request:

```
[ <cr><lf>
```

Example response:

```
[<cr><lf>
```

### **RS 485 Interface Commands**

The RS 485 Interface allows multiple sensors to be controlled from a single host over distances of several hundred feet. All devices as well as the host transmit and receive data over a single wire pair. Note that for distances greater than 10 feet, both ends of the cable should be terminated in the characteristic impedance of the line (typically 100 ohm).

The Protocol used by the RS485 Interface is identical to the TTL interface except for the addition of a “Select” command (!). The select command allows the host to specify which of the multiple devices attached to the line will respond to subsequent commands.

### *! Command – Select Device*

This command selects the device with the specified address. For device addresses other than 0, the device with the specified address will generate the response. All other devices remain silent. For device address 0, any device on the line will respond and will return its presently configured address. Note that when device address 0 is used any device select will reply with its address – only one device should be present on the line. This feature is intended solely for identification of the device address. The address is portion of parameter 4.

The following example selects device 5.

Example Request:

```
! 5<cr><lf>
```

Example Response:

```
! 00005<cr><lf>
```

Note that the address is provided in the response in the same format as other values, i.e. 0 to 65535 with leading zeros.

All devices will deselect when the ! character is received.

Example request:

```
!<cr><lf>
```

Example response:

```
No response
```

This assures that a device will not remain selected due to a communications error. Devices will be selected only upon receipt of their address or the 0 address.

Self-Identification, selecting address 0 (only 1 device connected) reports programmed address from parameter word 4.

Example Request;

Copyright © 2014-2018 CO2Meter, Inc. EC200 Rev O



```
! 0<cr> <lf>
```

Example response;

```
! 00005<cr><lf>
```

### *# Command– Restart*

Same as power cycle, all 32 parameters will be reloaded.

Example Request:

```
# 12345<cr><lf>
```

Example Response:

```
No response
```

## Chapter 3 : Configuration

### General

The sensor controller configuration is controlled by 32, 16-bit parameter values that are stored in the flash of the microcontroller. These parameters control how the analog front-end device is configured, how values are converted to concentration, and the characteristics of the communication interface.

### Parameter Summary

The following table provides a brief summary of the 32 parameters and their default settings. All parameters are 16 bit integers (Note that these defaults may not be appropriate for all sensor types).

#	Default Value	Name	Description
0	N/A	Checksum	This is a computed value used to verify integrity
1	4294	Output Mode	Bit Mask of Output Values,
2	0	Log Mode	Bit Mask of Logging Values if 0 no logging
3		Sensor AFE Config	AFE 91000; Low byte TIACN & Load, Hi byte REFCN source zero and bias. Default is sensor dependent.
4	05	Options Configuration	Configuration Option Word, ADR RS485, PWM
5	0	Log Interval	Interval between logs in seconds if 0 no logging
6	1	Gas Type	See Table of Gas Types below
7		Zero	ADC value corresponding to zero at 25C generated at calibration U command.
8		Calibration at Reference gas	ADC value corresponding to ref gas at 25C generated by the X command.
9		Calibration Concentration	Scaled concentration of reference gas ppm stored when X command is executed.
10		Full Scale PWM	Full scale value for PWM; typically, 25K PPM for O2 and 2k PPM for CO
11		Full Scale Analog	Full scale value for Analog out typically 25K for O2 and 2K for CO
12	1	Multiplier	Scale Multiplier in ppm sensor dependent.
13		Feature configuration	Bit 0 - Temperature compensation disabled when set. AFE from sensor and AUX PGA Gains 15-13 ADC 0, 12-10 ADC 1, 9-7 ADC 2. 0-5 active 6&7 invalid.
14-15		Reserved	

16-31		TC Values	16 Temperature Compensation Values

### Checksum (0)

The checksum is a computed value used to verify the integrity of the parameter data calculated W, U, X commands. On power up or # command, checksum for stored values is tested, if in error, default values (same as “w” command) are loaded and checksum set to 21930.

### Output Mode (1)

The Output Mode is a bit mask that specifies which measurements are output in streaming mode. The bit assignments are described in Chapter 3 under the “M” command. At power up default value is loaded. M command changes current mask, to set as default the W command is required,

### Log Mode (2)

The Log Mode is a bit mask that specifies which measurements are logged when logging is enabled. The log mode bit mask has same parameter definitions as Output Mode mask.

### AFE Configuration (3)

This parameter sets the configuration of the Analog Front End. The values depend on the electrical characteristics of the sensor. Configuration of the AFE is outside the scope of this document.

### Configuration Option Word (4)

The configuration option word sets various device options. These include the RS485 device address, the Polling Mode at power up. Values are scribed in Chapter 3 under the “K” command.

Config Options(s)	Default	Bit Value	Description
Streaming	Off	32768	When this bit is set the device will stream after power up. (Until changed by K command)
PWM/ Analog OUT	Off	16384	Enable PWM and Analog Pin 2 and 9
Reserved	Off	8192	
Reserved	Off	4096	
Reserved	Off	2048	
Reserved	Off	1024	-
Reserved	Off	512	-
Reserved	Off	256	-
Reserved	Off	128	-
Reserved	Off	64	-
Reserved	Off	32	-

Device Address	5	0-31	RS485 Device Address
----------------	---	------	----------------------

The configuration word is set by adding the bit values for each option. For example, to set the “Select Protocol Option” with a device address of 5, parameter 4 must be set to a value of 16389 (16384 + 5). Note that streaming should also be turned off when using the select protocol.

#### **Log Interval (5)**

This is the Interval between log entries in seconds. A value of zero will disable logging.

#### **Gas Type (6)**

This is the type of gas. The values are as follows:

Value	Abbreviation	Gas Species
0	UNK	Unknown
1	CO	Carbon Monoxide
2	O2	Oxygen
3	H2S	Hydrogen Sulfide
4	NH3	Ammonia
5	ET	Ethylene C2H4
6	CL2	Chlorine
7	N2O	Nitrous Oxide
8	SO2	Sulfur Dioxide
9	NO2	Nitrogen Dioxide
10	EtO	Ethylene Oxide
11	HCL	Hydrogen Chloride
12	O3	Ozone
13	User define	
15	User Define	

#### **Zero Calibration (7)**

This is the ADC value at zero calibration.

#### **Calibration at Reference (8)**

This is the ADC value at the reference calibration concentration.

#### **Calibration Concentration (9)**

This is the concentration at which calibration was performed save for reference..

#### **PWM Full Scale (10)**

Full scale range for 100% PWM typically 25K for O2 and 2K for CO. 20.9K PPM/25K PPM= 83.6 % Full scale PWM.

### Analog Full Scale (11)

Full scale range for 100% Analog (3 volts) typically 25K for O2 and 2K for CO. 20.9K PPM/25K PPM= 83.6 % Full scale = 2.508 volts..

### Multiplier (12)

This is the multiplier value to arrive at ppm from the specified values. A value of 0 indicates that readings are in tenths of ppm. 1 indicates 1 ppm, 2 indicates 10ppm, 3 indicates 100ppm etc.

### Feature Configuration (13)

Value for configuration of AFE PGA's and other selectable functions.

Config Feature Parameter 13	Default	Bit Value	Description
Gain AFE CH0 PGA	000	32768 16384 8192	Input from 91000 C2 CH0 ADC voltage millivolts
Gain AFE CH1	000	4096 2048 1024	Input from 91000 Vout CH1 ADC voltage millivolts
Gain AFE CH2	000	512 256 128	Auxiliary differential input. Note that each of these inputs must be referenced to ground within the common mode range of the input values ( -1V to +2.8V).
Reserved		64	
Reserved		32	
Reserved		16	
Reserved		8	
Reserved		4	-
Pressure compensation		2	When = 1 enables pressure compensation
Temperature compensation	0	1	When = 1 disables gas sensor temperature compensation

The AFE Gain bit values are:

- 000 Gain of 1 (Default)
- 001 Gain of 2
- 010 Gain of 4
- 011 Gain of 8
- 100 Gain of 16
- 101 Gain of 32
- 110 Invalid - Do Not Use
- 111 Invalid - Do Not Use

For example, to set the gain to 8 for channel 2 (9,8,7) the gain value must be 011, i.e. bits 8 and 7 must be on. This requires a decimal value of 256 + 128 or 384 be added for this word from the default of 0).

So to program this the sequence.

Example; get the current value for reference

```
command: p 13 <cr> <lf>
```

```
response: p 13 00000
```

Set the value to 384

```
command: P 13 384
```

```
response: P 13 384
```

Write parameters to flash

```
command: W
```

```
response: W
```

Software reset to reload new gain value

```
command: # 12345
```

### ***Temperature Compensation Values (16-31)***

These are 16 temperature compensation values that range from -30C to 45C in 5 degree C increments. These values are correction factors in unsigned Q14 format. In this format 32768 corresponds to 1, 32769 is 1 plus 1/32768.

The default values for these numbers is set to typical correction factors for the particular type of sensor. When auto calibration is performed, these values are set to match the actual characteristics of the particular sensor.

A null table no temperature corrects, would be parameters 16-31 =32768

## Chapter 4 : Calibration

**WARNING:** When performing calibration from reference gas always consult the Material Safety Data Sheet for the gas specie and concentration in use and observe all relevant safety precautions.

### General

Electrochemical sensors produce a current output that is linearly proportional to the gas concentration. While extremely linear, the output level varies from sensor to sensor and from batch to batch. In order to provide an accurate output, the sensor and its controller electronics must be calibrated. Generally, this requires an accurate zero point and a second calibration point with a known gas calibration.

Although the sensor output is linear, the chemical reaction that produces the output is sensitive to temperature. This sensitivity varies with temperature and varies from batch to batch and sensor to sensor. In order to provide an accurate reading, it is necessary to compensate for this temperature sensitivity. The EC200 provides the capability to automatically save these compensation values during an automatic calibration process.

### Basic Calibration

Basic Calibration requires first that an accurate zero be set (typically with Nitrogen Gas at 25C +/- 1C) and then that a known gas concentration be provided (also at 25C +/- 1C) and allowed to completely stabilize.

The zero-calibration point is set using the U command. The reference point is set using the X command. When the X command is executed the microcontroller makes the necessary calculations for full span and stores these in the parameter storage.

By default, the temperature compensation values are set to typical values for the type of sensor involved. These typical values are sufficient for most applications. If the highest accuracy is desired, the automatic calibration mode can be used to capture the temperature compensation values for the particular sensor cell installed.

### Recommendation handling, storage and calibration;

EC sensor are allowed temperature stabilize before calibration, particularly if sensors are stored refrigerated.

Sensor being store ambient or refrigerated should be shorted to prevent polarization. Sensor stored un-shortened for long periods, should be shorted or mounted and allowed to normalize ~60 min. The EC200 sensor board have an internal shorting mechanism. Calibrate to the application target or threshold, using calibration gas always check the expiration date of the gas.

Nitrogen for zero, consider the application, gas with low target threshold like CO (9 ppm background typical) for precision work a 99.999% should be use.



## Chapter 5 : Logging

### General

The EC200 equipped with 64K Bytes of logging memory. This can be used to log from 1 to 12 values at intervals of 1 second to 12 hours. Logs can be retrieved via the serial interface.

### Log Blocks

The 64K bytes of logging memory are divided into 128 blocks (512 bytes each). The last block is reserved for recording information about the calibration. The remaining 127 blocks are used for log storage.

Each block is 256 words in length. Each block begins with a date/time stamp that is 4 words in length. This is followed by the log interval in seconds and the log mask. The log mask has a bit for each value that is logged. The number of bits that are set determines the length of each log record.

The remaining 250 words in the block contain log records, each a fixed length in words equal to the number of measurements that are logged. The entire block contains, at most, whatever number of records will completely fit in the block. For example, if only the gas concentration (Z) is logged, then the block can hold up to 250 records. If 12 measurements are logged, a block will hold 20 records (240 words) and the last 10 words of the block will remain unused. Unused log entries will always contain 65535 (0xffff hex).

### Short Blocks

Each time the unit is powered up, or the log parameters are changed, or the date/time is changed, the current block is immediately closed and new log block will be started reflected the new values. The end of a short block is always indicated by a value of 65535 (0xffff).

### Log Capacity

The total capacity of the log ranges from 31750 entries if only a single measurement is logged to 2540 entries if all 12 measurements are logged. Logging Gas Concentration, Temperature, Relative Humidity, and Barometric pressure (4 readings) the log will hold 7874 records. With an interval of 6 minutes, the log will hold more than a month of readings.

### Date/Time Format

The first 4 words of each block contain the date/time of the first record written to the block. This data is in the native format of clock calendar device used on the controller. The data consist of 8 bytes in little-endian order, i.e. the least significant byte of the word is first.

- Byte 0 is seconds in BCD (binary code decimal) .
- Byte 1 is minutes in BCD.
- Byte 2 is hours in BCD on a 24 hour clock.

- Byte 3 is the day in BCD
- Byte 4 is not used and should be ignored.
- Byte 5 is the month in BCD
- Byte 6 is the last two digits of the year in BCD

Note that in BCD two decimal digits are encoded per byte, each with a 4 bit binary value that ranges from 0 to 9.

### Block header decoding start time example;

Example request: Get first 6 words from start of block, i.e. 0, 256, 512;

```
R 0 6 <cr> <lf>
```

Example receive: 6 integer decimal values;

```
RECV:r 20773 01554 01024 65304 00005 15424
```

Convert time and date words Decimal- Hex integer- Packed BCD  
5125 0612 0400 FF18

51 Minutes  
25 Seconds  
12 Hour (24 hour)  
06 Day  
00 unused  
04 Month  
FF unused  
18 Year

00005 logging interval in second.

15424 Mask for field to log.

### Example of logging operation, partial block and start restart;

Set logging interval to 4 seconds start logging

```
SEND:P 5 4
```

```
RECV:P 00005 00004
```

Set logging interval to 0; stop logging

```
SEND:P 5 0
```

```
RECV:P 00005 00000
```

Read 100 word starting at 0;

```
SEND:R 0 100
```

Note; time and date and interval of 4 seconds and logging mask 4294

```
RECV:r 01540 05397 00513 65304 00004 04294 00001 0002  
RECV:r 01232 12088 00541 00003 00002 01232 12089 0540  
RECV:r 00003 00002 01232 12090 00544 00001 00002 1234  
RECV:r 12087 00555 00003 00001 01235 12087 00552 0002  
RECV:r 00002 01235 12089 00548 00002 00002 01235 2089  
RECV:r 00545 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 5535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 5535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 5535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:R 65535 65535 65535 65535
```

Restart logging at 7 second interval.

```
SEND: P 5 7
```

```
RECV: P 00005 00007
```

Stop logging

```
SEND: P 5 0
```

```
RECV: P 00005 00000
```

Read 100 words starting at 0- 100

```
SEND:R 0 100
```

```
RECV:r 01540 05397 00513 65304 00004 04294 00001 00002  
RECV:r 01232 12088 00541 00003 00002 01232 12089 00540  
RECV:r 00003 00002 01232 12090 00544 00001 00002 01234  
RECV:r 12087 00555 00003 00001 01235 12087 00552 00002  
RECV:r 00002 01235 12089 00548 00002 00002 01235 12089  
RECV:r 00545 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:R 65535 65535 65535 65535
```

Read 100 word starting at 256 – beginning of next block

```
SEND:R 256 100
```

Note restart of logging time and date and new interval of 7 second;

```
RECV:r 01842 05397 00513 65304 00007 04294 00001 00001  
RECV:r 01237 12087 00528 00003 00002 01237 12087 00529  
RECV:r 00001 00002 01239 12087 00544 00003 00002 01241  
RECV:r 12090 00544 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:r 65535 65535 65535 65535 65535 65535 65535 65535  
RECV:R 65535 65535 65535 65535
```

## Support

The quickest way to obtain technical support is via email. Please send all support inquiries to [support@co2meter.com](mailto:support@co2meter.com).

Please include a clear, concise definition of the problem and any relevant troubleshooting information or steps taken so far, so we can duplicate the problem and quickly respond to your inquiry.

## Warranty

This device comes with a 90 day (warranty period) limited manufacturer's warranty, starting from the date the meter was shipped to the buyer.

During this period of time, CO2Meter.com warrants our products to be free from defects in materials and workmanship when used for their intended purpose and agrees to fix or replace (at our discretion) any part or product that fails under normal use. To take advantage of this warranty, the product must be returned to CO2Meter.com at your expense. If, after examination, we determine the product is defective, we will repair or replace it at no additional cost to you.

This warranty does not cover any products that have been subjected to misuse, neglect, accident, modifications or repairs by you or by a third party. No employee or reseller of CO2Meter.com's products may alter this warranty verbally or in writing.

## Liability

All liabilities under this agreement shall be limited to the actual cost of the product paid to CO2Meter.com. In no event shall CO2Meter.com be liable for any incidental or consequential damages, lost profits, loss of time, lost sales or loss or damage to data, injury to person or personal property or any other indirect damages as the result of use of our products.

## Returns

If the product fails under normal use during the warranty period, a RMA (Return Material Authorization) number must be obtained from CO2Meter.com. After the item is received CO2Meter.com will repair or replace the item at our discretion.

To obtain a RMA number, call us at or email us at (386) 256-4910 [support@co2meter.com](mailto:support@co2meter.com).

When requesting a RMA please provide reason for return and original order number. If we determine that the product failed because of improper use (water damage, dropping, tampering, electrical damage etc.), or if it is beyond the warranty date, we will inform you of the cost to fix or replace the product.

For more information visit our website: [www.CO2Meter.com/pages/faq](http://www.CO2Meter.com/pages/faq)

## Contact Us

### We are here to help!

For information or technical support, please contact us.

✉ [support@co2meter.com](mailto:support@co2meter.com)

☎ (386) 256-4910 ( Technical Support)

☎ (386) 872-7665 (Sales)

🌐 [www.co2meter.com](http://www.co2meter.com)

Address:

CO2Meter, Inc.

131 Business Center Drive

Ormond Beach, FL 32174

USA